

FIG. 1
(PRIOR ART)

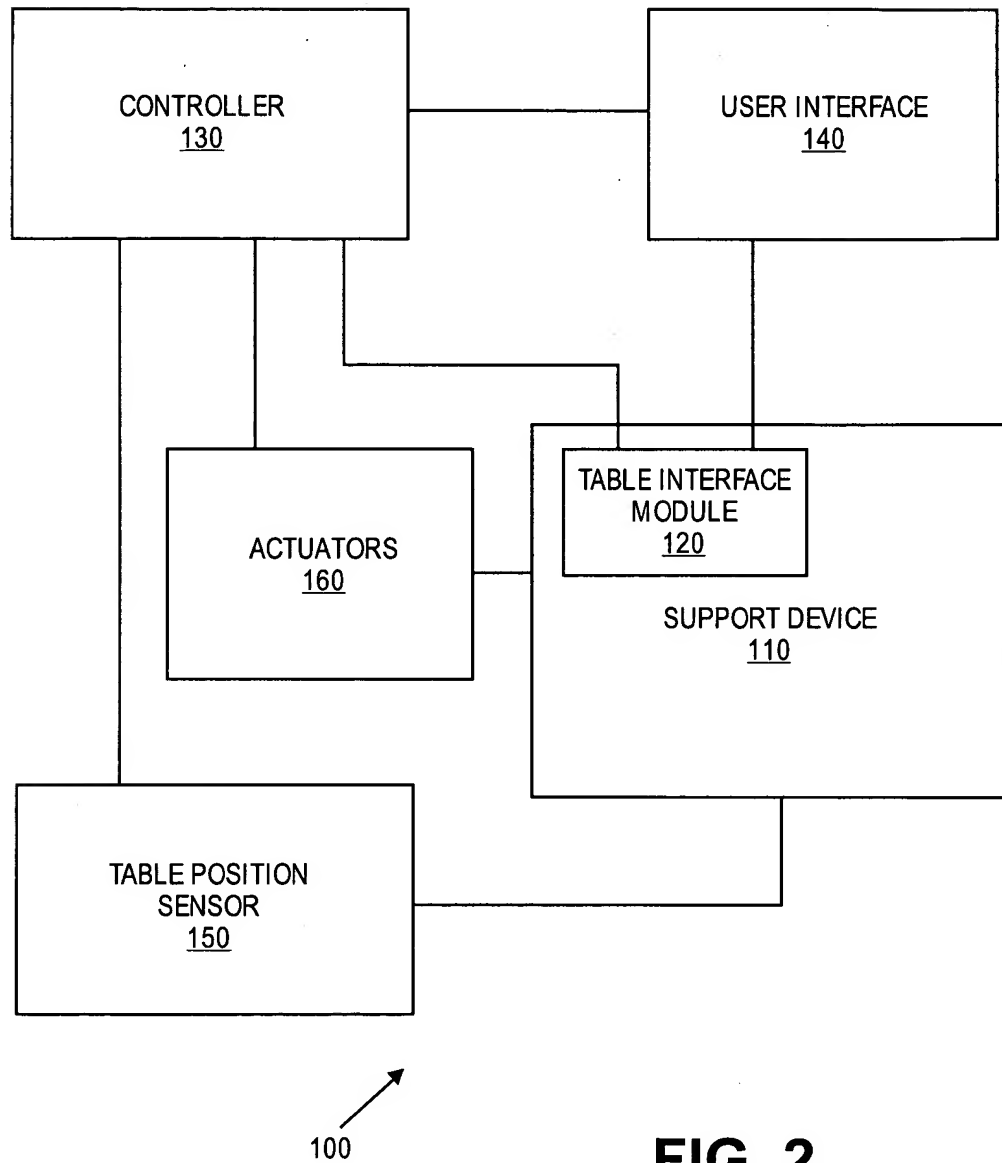


FIG. 2

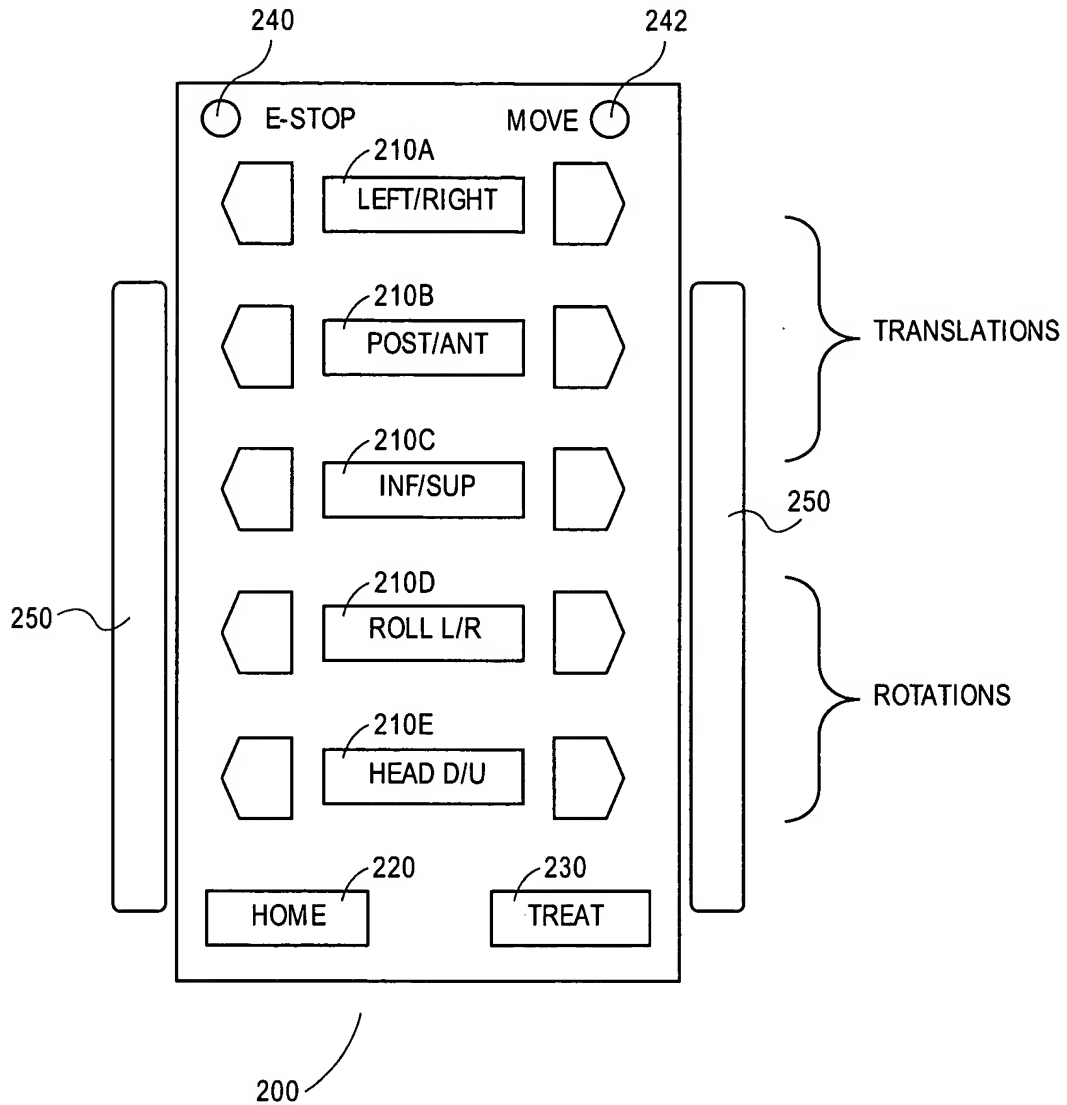


FIG. 3

FIG. 4

FIG. 4

310

320

330

400

AUTOCOUCH ALIGNMENT DIALOG

TREATMENT DATA

NAME: BICRON_FIDUCIAL_P
MEDICAL ID: 021202
PHYSICIANS: ME
ACQUIRE

CONTROLS

☐ MANUAL ALIGNMENT
☐ TRANSLATIONS
☐ ROTATIONS
MOVE
☐ USEROTATIONS

TRANSLATIONS

INF(+)/SUP(-) [0.3] ROLL-L(-)/R(+) [-0.1]
LEFT(+)/RIGHT(-) [1.0] HU(+)/HD(-) [-0.1]
ANTI(+)/POST(-) [1.5] COW(+)/CW(-) [0.6]

ALIGNMENT CRITERIA

MAX NO. OF MOVEMENTS [6]
MAX TRANSLATION [2.0]
MAX ROTATION [0.5]

ALIGN **CANCEL**

AUTOMATIC ALIGNMENT

ANT LFT RGT

TRACKING MODE

SKULL TRACKING 6D
X-RAY PARAMETERS
Patient Alignment

FIDUCIAL TRACKING

FIDUCIAL AREA
SEARCH
IDENTIFY
TRACK
TRACKING MODE

VIEW MODE

X-Hairs
DISPLAY-FIDUCIAL MARKERS
DISPLAY-ROI
THRESHOLD

STATUS BAR

XRS A KV: 120 MA: 100 EX: 50 WINDOW: 0 LEVEL: 0
XRS B KV: 120 MA: 100 EX: 50 WINDOW: 255 LEVEL: 210
XRS C KV: 120 MA: 100 EX: 50 WINDOW: 255 LEVEL: 210